



НҮҮРСНИЙ ОВООЛГЫН ҮЗҮҮЛЭЛТ

№ ETT_SP_CC



ISO 45001:2018



ISO 9001:2015



ISO 14001:2015



НҮҮРСНИЙ ОВООЛГЫН ЧАНАРЫН ДУНДАЖ ҮЗҮҮЛЭЛТ

ДОТООД ЧИЙГ (ad)

1.0%

max

ҮНСЛЭГ (db)

13.0%

(-3.0; +3.0)

ДЭГДЭМХИЙ (daf)

26.0%

(-2.0; +2.0)

НИЙТ ХҮХЭР (ad)

≤1.5%

БАРЬЦАЛДАХ ЧАНАР

≥75.0

НҮҮРСНИЙ ХЭМЖЭЭ

416.0

МЯН.ТН

НҮҮРСНИЙ ОВООЛГЫН ШИНЖИЛГЭЭНИЙ ҮР ДҮН

ALS GROUP LLC
Mongol National Building, 2nd Floor
Chinggis Avenue, Khan-Uul District
Ulaanbaatar, Mongolia
Tel: +976 70007647



CLIENT: Erdenes Tavan Tolgoi JSC
ADDRESS: Finance Center, Jigjidiya 8
1st khoroо, Chinggis Avenue
Ulaanbaatar, Mongolia
ATTN: Bilguunmaali
PROJECT NO. xxx
LAB. JOB NO. 23002, 05, 14, 24, 31, 47, 51, 52, 56, 62-TT
NO. SAMPLES: 30
Notes/Comments: xxx

CERTIFICATE OF ANALYSIS

23002, 05, 14, 24, 31, 47, 51, 52, 56, 62-TT


SAMPLES RECEIVED: 08-01/07/2023
INSTRUCTIONS RECEIVED: 08-01/07/2023
DATE OF REPORT: 08-02/07/2023
STATUS OF REPORT: FINAL
ANALYSIS COMPLETE: 08-02/07/2023
PREPARATION CODE: CRUSH 01, 02: MILL 01
ANALYSIS CODE: 1_COOKING COAL_CSN
TM, ASH, MOIS, VOL,
TSUL, CSH, CSN

APPROVED BY: Laboratory Manager



These test results are representative only of the sample received in the laboratory.

Table with columns for STANDARD METHOD, LAB NO., SAMPLE NO., and various chemical analysis results (Total Moisture, Ash, Volatile Matter, Fixed Carbon, Total Sulphur, Moisture, Ash, Volatile Matter, Fixed Carbon, Total Sulphur) for AS RECEIVED BASIS, AIR DRIED BASIS, DRY BASIS, and DRY, ASH-FREE BASIS. Includes a sub-table for QUALITY ASSURANCE/QUALITY CONTROL DATA.

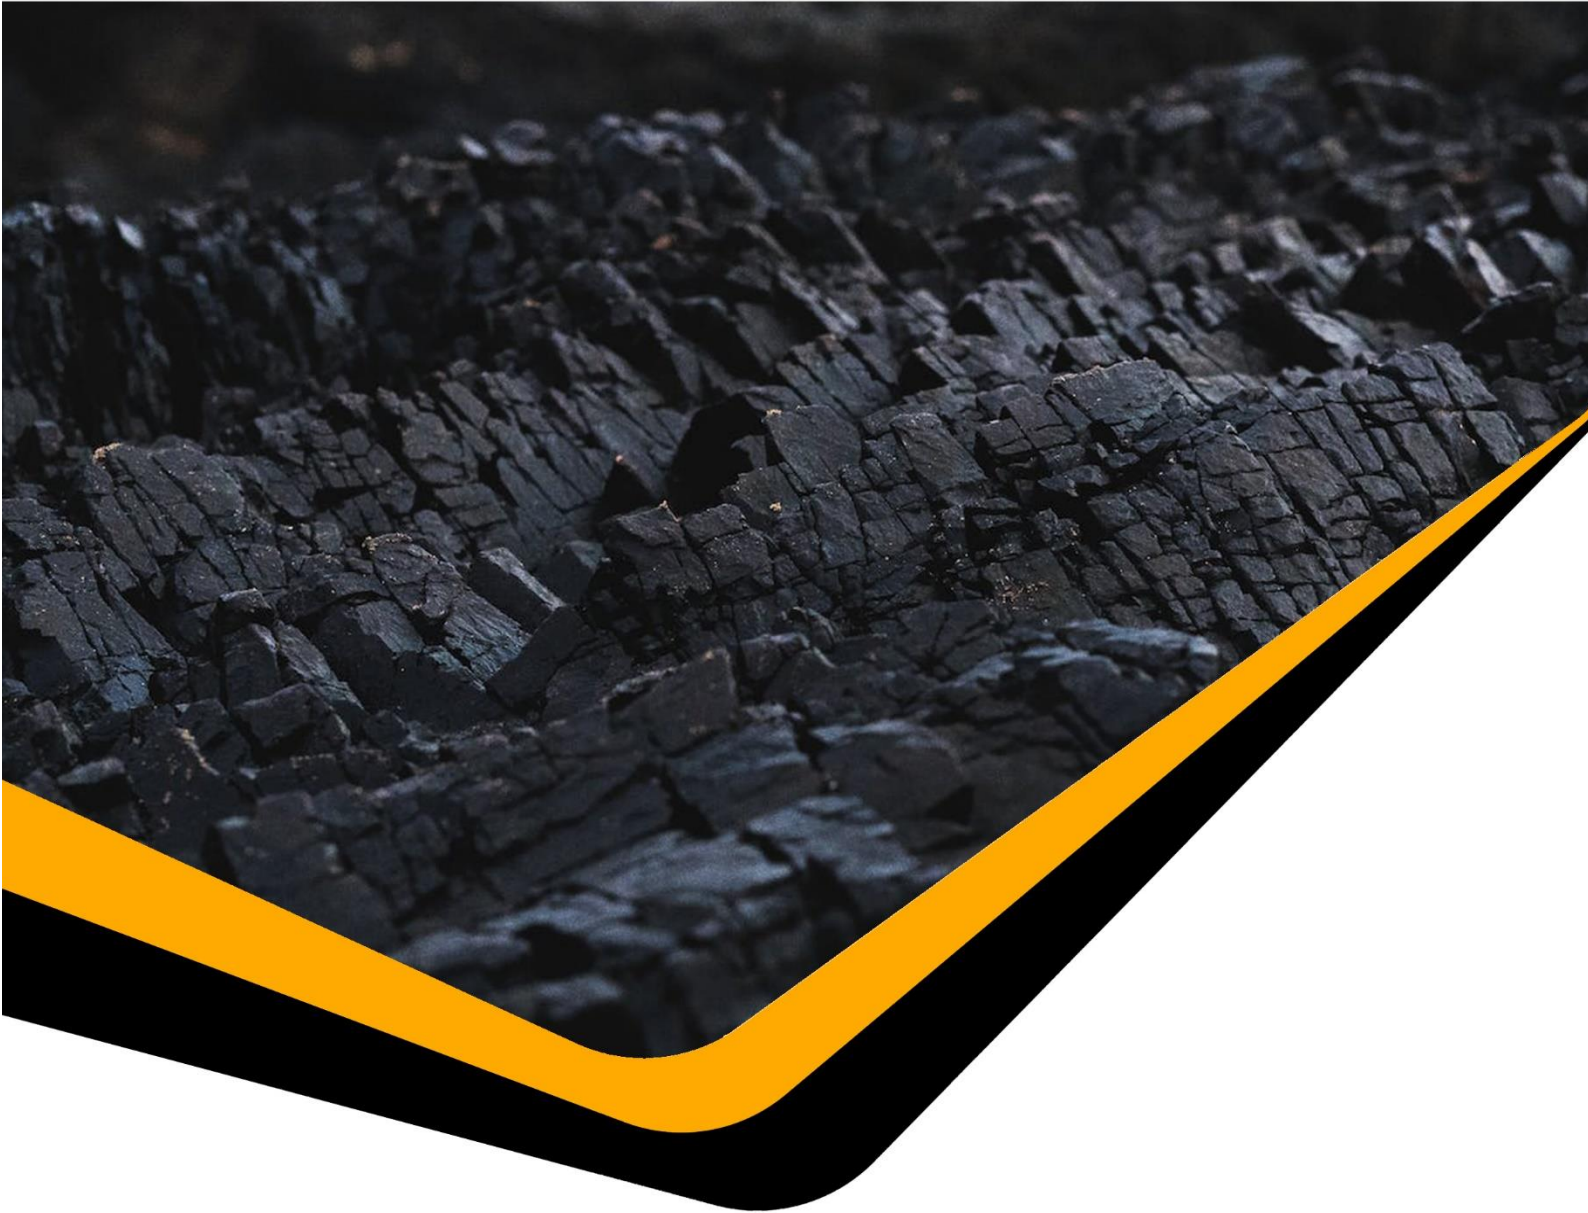

ISO 45001:2018



ISO 9001:2015



ISO 14001:2015



www.ett.mn



75055555
1800-1072



Финанс төв, 1-р хороо,
Чингэлтэй дүүрэг,
Улаанбаатар хот

